

Smart Contact Lens Monitors Blood Sugar

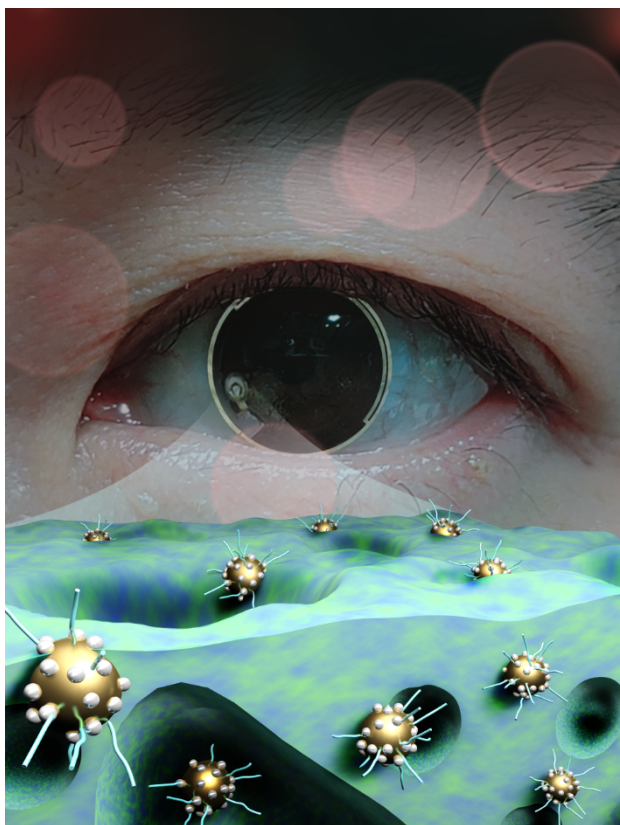


Image credit, Geon-Hui Lee

By [Andrew Myers](#)

It is said a tear is an insight into a soul, but soon it could reveal multitudes about a person's body chemistry, too. Researchers at Stanford University and POSTECH have developed a smart contact lens that quickly, accurately and *continually* monitors a person's blood sugar.

If approved and commercialized, such lenses could have a "huge" clinical impact, the authors say in a paper published in the journal *Advanced Materials*. The smart lens holds the promise of not only continuous, non-invasive monitoring for hypoglycemia and hyperglycemia, but of delivering alerts and perhaps even treatments anytime blood sugar goes awry. As such, they stand to help tens-of-millions of people worldwide avoid dangerous, possibly fatal, side effects of high or low blood sugar — tremors, confusion, epileptic seizure, and coma.

Chemistry is knowledge

In the rapidly emerging field of wearable biometric devices, the glucose monitoring contact lens employs a clever combination of existing and cutting-edge technologies. Existing glucose detection devices worn on or just under the skin typically employ electrochemical sensors and a glucose-metabolizing enzyme—glucose oxidase—embedded in the wearable material.

The engineers have succeeded with the addition of gold and platinum nanoparticles embedded in the polymer hydrogel that forms the contact lens. These hydrogels are porous. They absorb glucose-containing tear fluid from the eye surface and perform a simple chemical reaction. The gold and platinum serve as catalysts, expediting a reaction without getting used up themselves.



Image credit, Geon-Hui Lee

The engineers modified the gold and platinum particles adding hyaluronic acid that increases their distribution and long-term stability in the hydrogel. Likewise, the team fine-tuned the degree of porosity in the hydrogel. Tears are a precious commodity. Only a thin layer coats the eye. It's a delicate balance. If the hydrogel is too porous, the structural integrity of the lens might be compromised. If it's too impermeable, the lens might fail to absorb enough tear for successful measurement.

Correctly engineered, however, the smart contact plays host to a multistep chemical reaction. At its most basic level, glucose in the tear undergoes a chemical reaction in the hydrogel that produces electricity. Circuits integrated in the lens then measure the strength of the electrical current and use it to calculate the amount of glucose in the tear—and by extension the blood.

In technical terms, the chemical flavin adenine dinucleotide (FAD) from the enzyme reacts with the glucose in the tear to produce $FADH_2$, among other chemical byproducts. $FADH_2$ then reacts with oxygen, producing H_2O_2 (hydrogen peroxide). At this point the gold-platinum nanocatalyst comes into

play, helping to split the H_2O_2 into its constituent elements, hydrogen and oxygen. Most critically, however, this splitting of hydrogen peroxide also releases two electrons. That is, it produces electricity.

The electrons are conducted through the lens to an electrode sensor that calculates the amount of glucose in the blood. The strength of that electrical current is in direct proportion to the amount of glucose in the tear, which in turn is proportional to the amount of glucose in the blood—more electricity means more glucose. Measurement data are then transferred wirelessly from the lens to a smartphone.

Stability and accuracy

The eWEAR smart contacts are not the first wearable blood sugar monitoring system. There are sensors that can be worn on or embedded just under the skin, for instance. There have even been other contact lens approaches. But all have struggled to deliver accurate and consistent results over relatively long periods of time required of wearable devices. The smart contact is the first glucose monitoring device to make a direct correlation between tear and blood glucose concentrations independently without the aid of another medical device, such as a glucometer.

Other continuous monitoring systems have, so far, been hindered by technical challenges, including poor stability of the enzyme, low or inconsistent sensitivity of the glucose sensors, the relatively low volume of tears with which to work, slow absorption of tears into the lens polymer for processing, and slow diffusion of the chemicals produced during the reaction. Subcutaneous sensors are also prone to corrosion. To date, it has all added up to a lot of promise, without much punch.

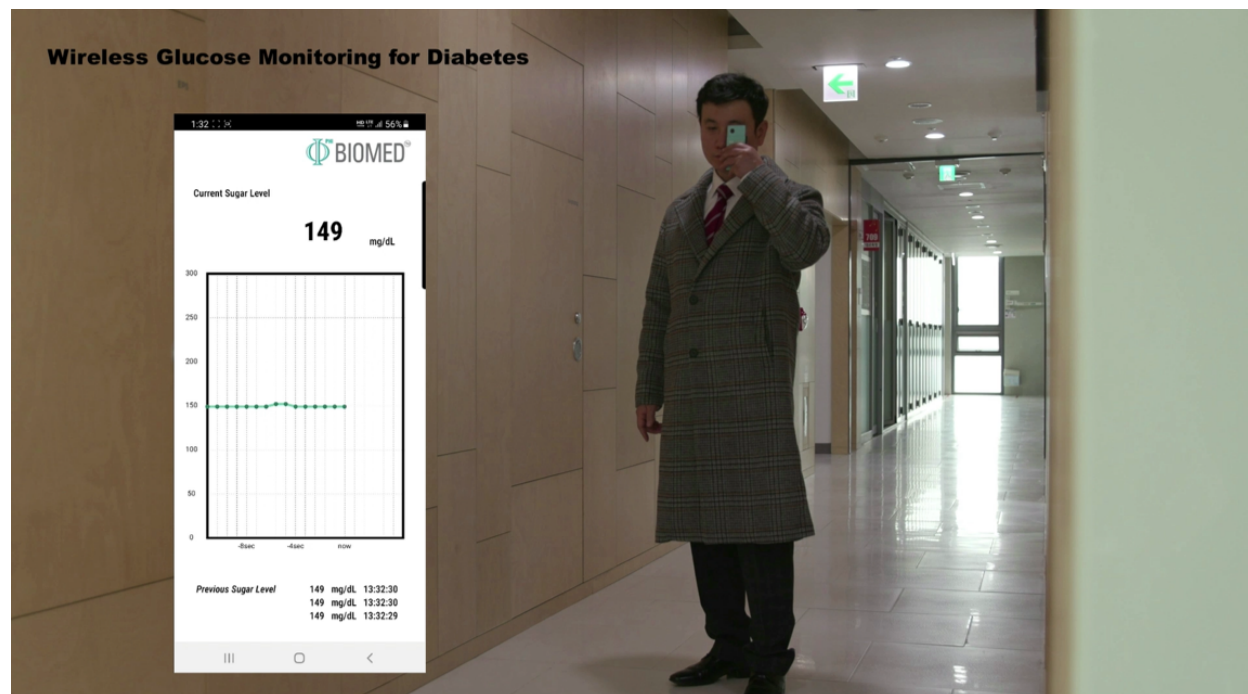


Image credit, Geon-Hui Lee

The authors credit the improved porosity in their hydrogel with increasing diffusion of the reaction chemistry through the device. This improves sensitivity considerably, cutting response time by almost half and lowering by ten times the threshold at which glucose can be detected—all positive

developments. Meanwhile, the addition of nanocatalysts greatly improves the crucial hydrogen peroxide-splitting reaction.

The researchers have tested their smart lens in rabbits ... and in a human. A volunteer from the research team served as a clinical trial of one. Results from those tests were at least as accurate as those made with a traditional glucometer, the authors say, reaffirming the promising feasibility of this smart contact lens in further clinical applications.

*The research team comprised a multi-institutional corps of researchers including authors **Zhenan Bao** and **David Myung** of the Department of Chemical Engineering at Stanford University; **Cheonhoo Jeon** and **J.-Y. Sim** of the Department of Electrical Engineering at Pohang University of Science and Technology (POSTECH) in South Korea; **Su-Kyoung Kim**, **Geon-Hui Lee**, **Hye Hyeon Han**, **Seong-Jong Kim**, and **Sei Kwang Hahn** of the Department of Materials Science and Engineering at POSTECH; **Jee Won Mok** and **Choun-Ki Joo** of the Department of Ophthalmology and Visual Science at The Catholic University of Korea in Seoul; and **Sangbaie Shin** and **Sei Kwang Hahn** of PHI BIOMED Co. in South Korea.*

*The **eWEAR-TCCI awards for science writing** is a project commissioned by the Wearable Electronics Initiative (eWEAR) at Stanford University and made possible by funding through eWEAR industrial affiliates program member Shanda Group and the Tianqiao and Chrissy Chen Institute (TCCI®).*